

FIG.2

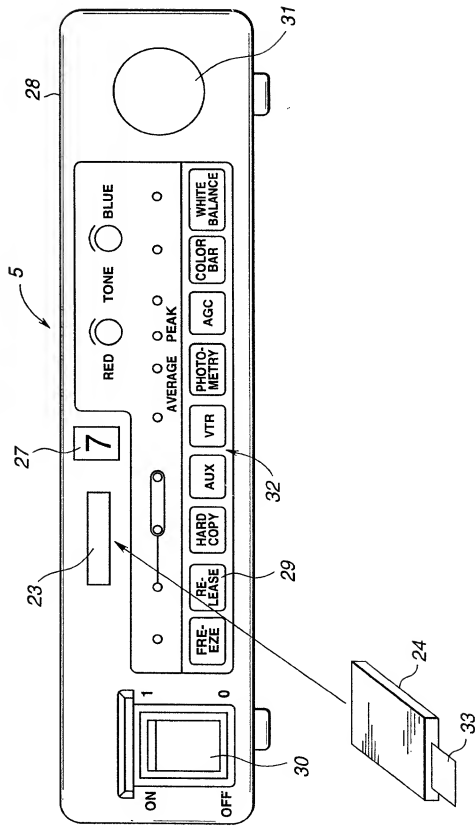
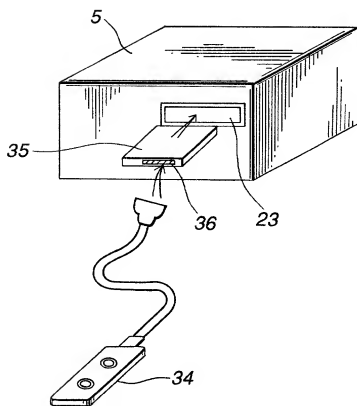


FIG.3



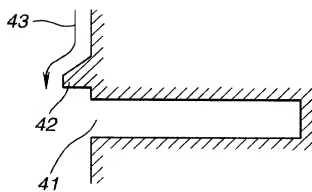
[illegible]

FIG.6

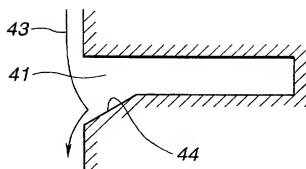


FIG.7

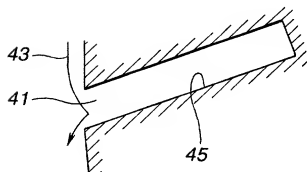


FIG.8

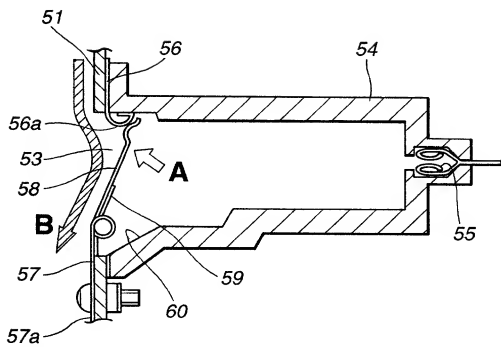


FIG.9




FIG.11





FIG.12



FACE

BACK

FIG.13

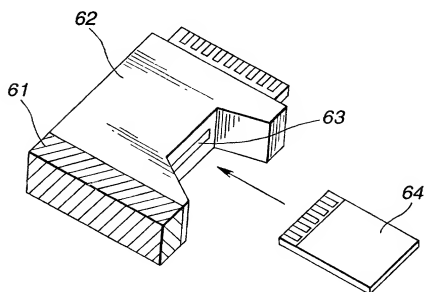


FIG.18

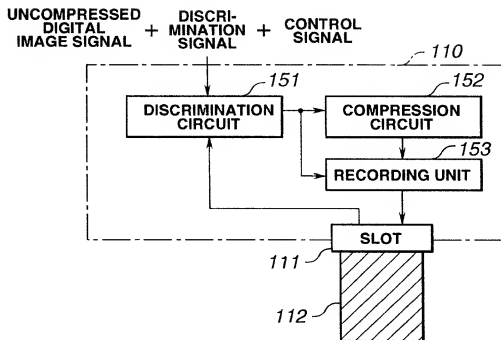


FIG.19

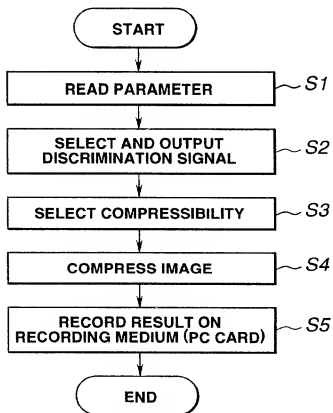


FIG.20

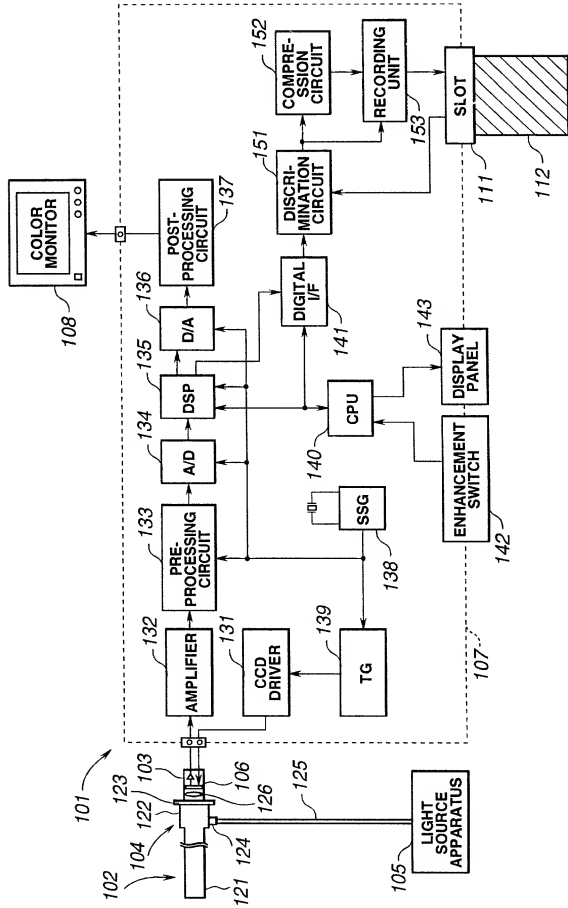


FIG.21

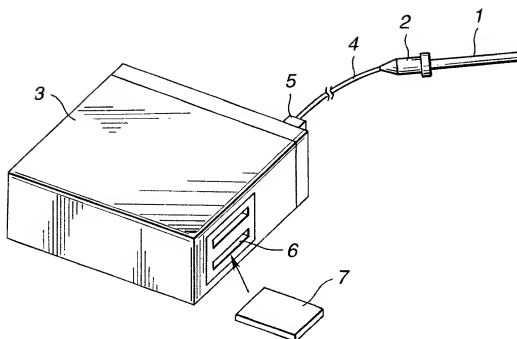


FIG.22

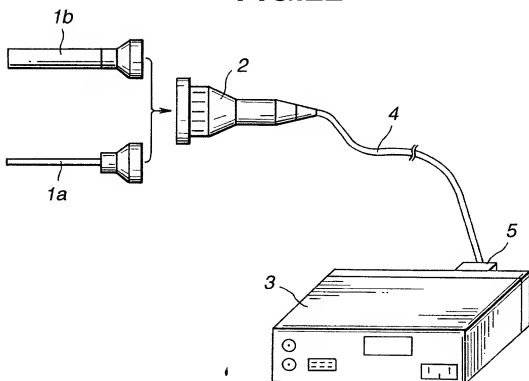


FIG.23

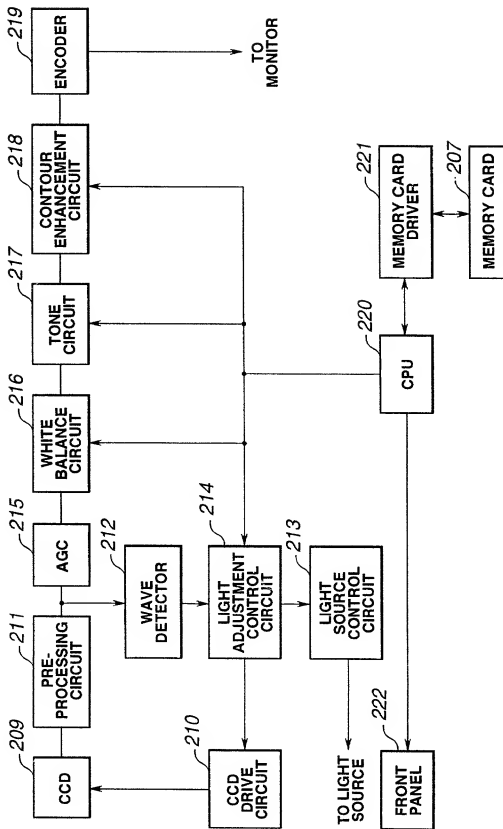


FIG.24

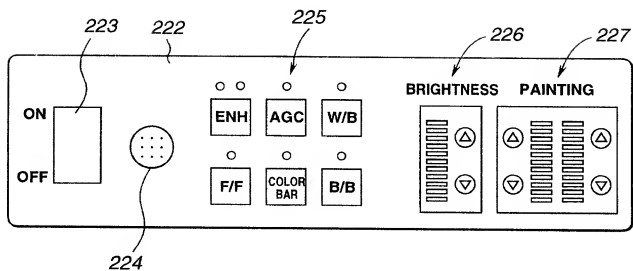


FIG.25

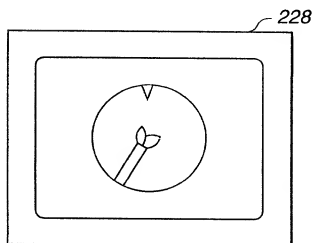


FIG.26

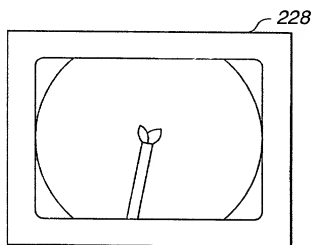


FIG.27

	LIGHT ADJUSTMENT		TONE	CONTOUR ENHANCE- MENT
	SPEED	LEVEL		
URETEROSCOPE/ ARTHROSCOPE	LOW	LOW	BLUISH	HIGH
LAPAROSCOPE	HIGH	HIGH	REDDISH	LOW

FIG.29

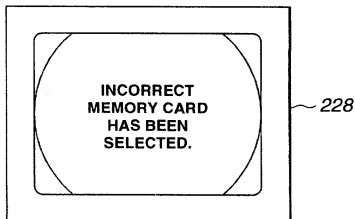


FIG.28

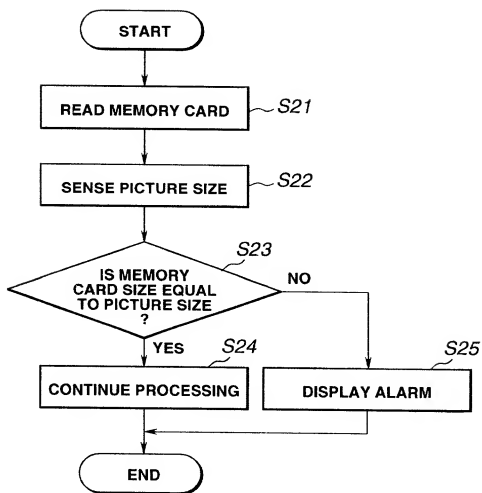


FIG.30




FIG.31




FIG.46
PRIOR ART

MENU		
<u>DR.1</u>	DR.2	DR.3
COLOR	R	<input type="text"/>
	G	<input type="text"/>
	B	<input type="text"/>
BRT		<input type="text"/>

FIG. 32

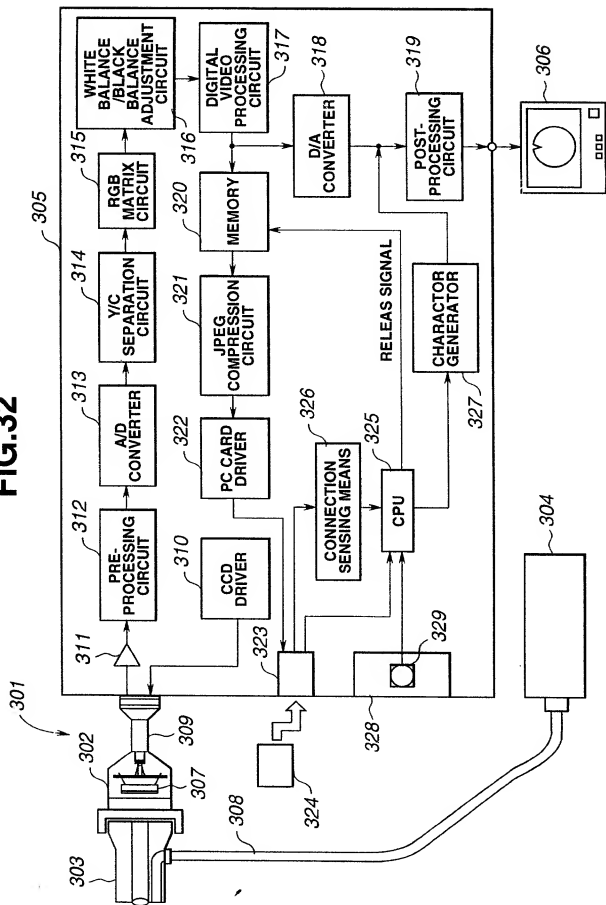


FIG. 33

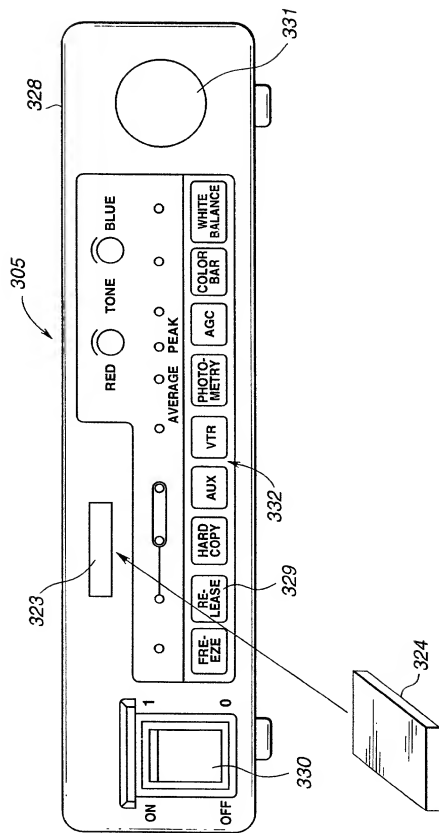


FIG.34




FIG.35

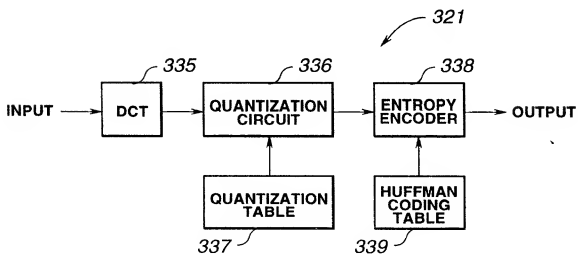


FIG.36

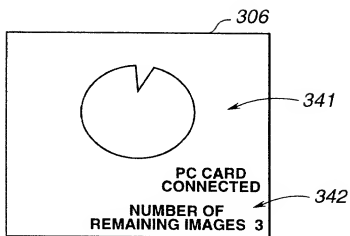


FIG.38

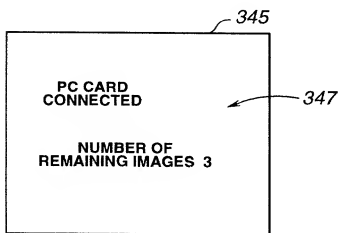


FIG.37

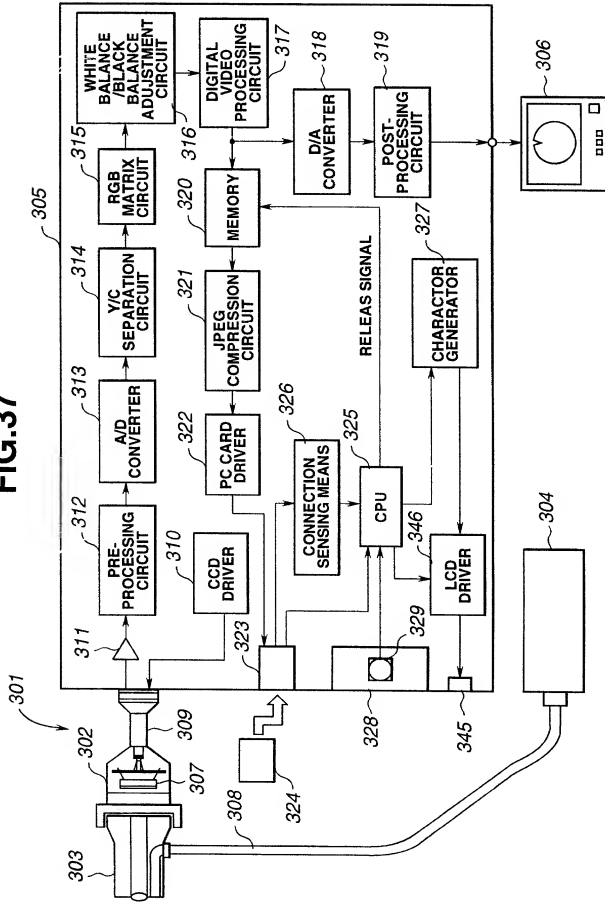


FIG.39

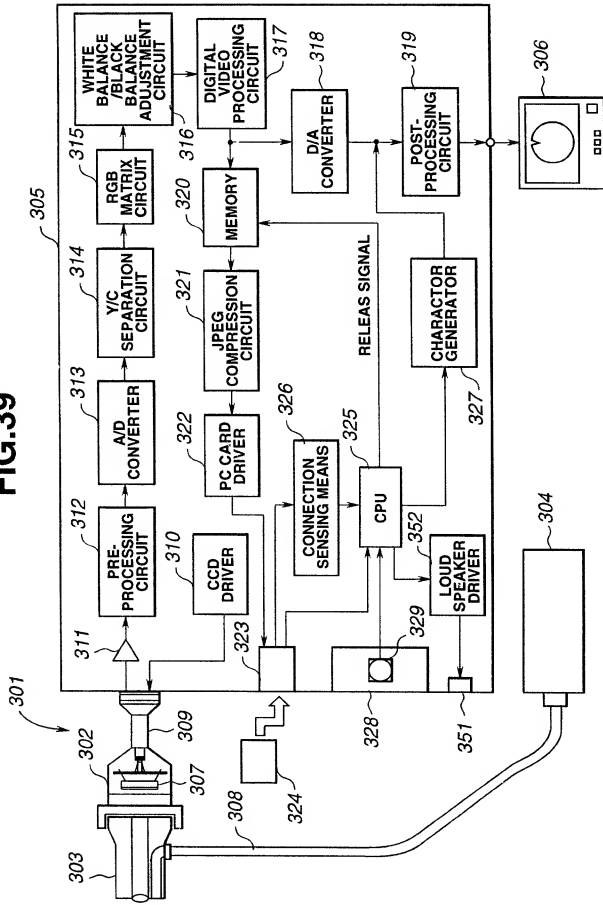


FIG.40

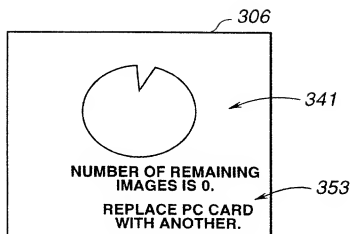
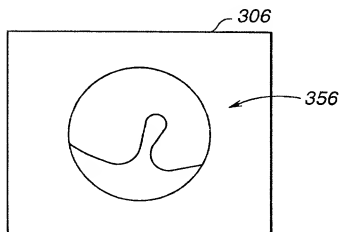


FIG.42



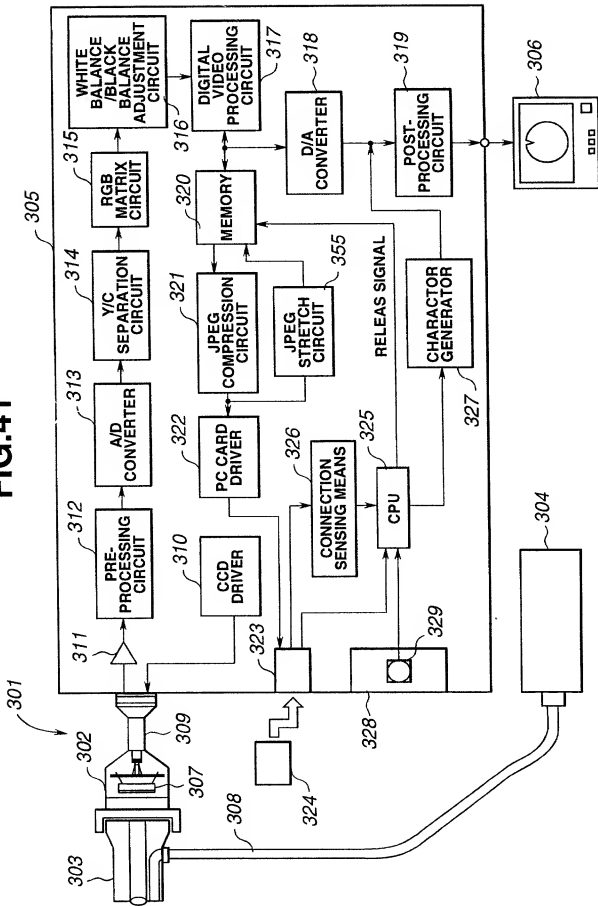


FIG.43

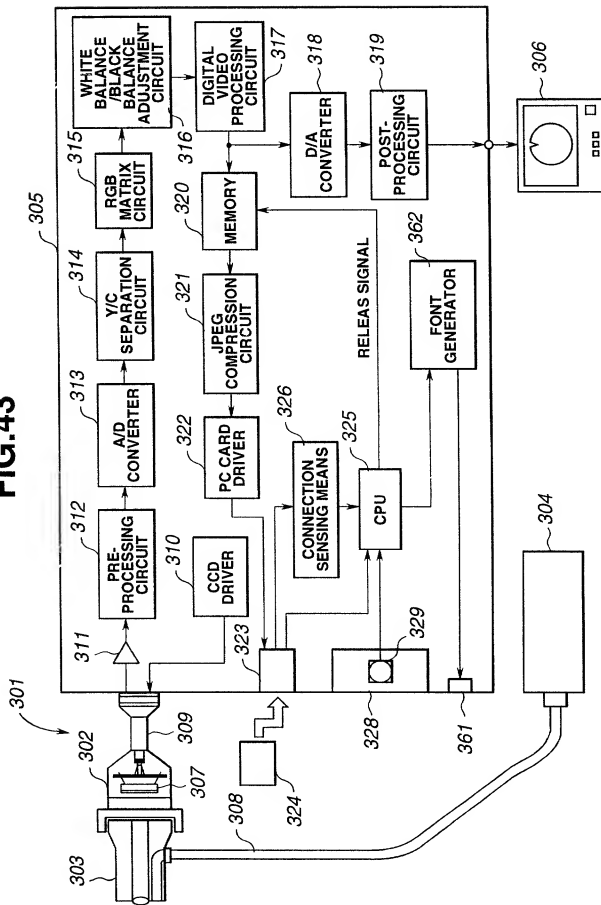


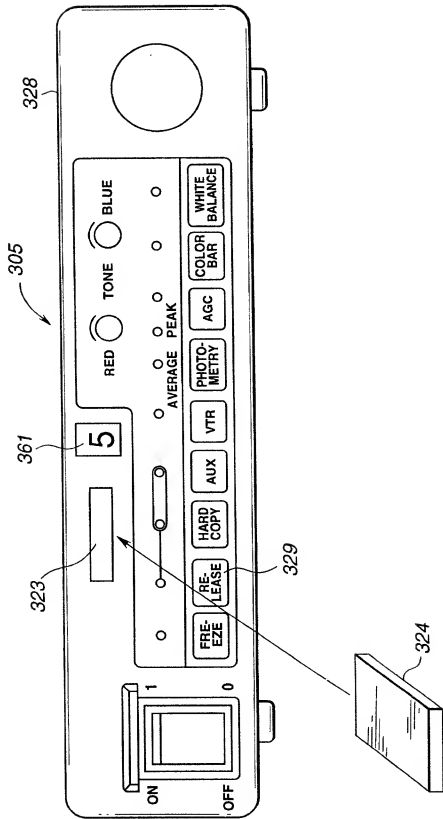
FIG. 44

FIG.45
PRIOR ART

